pH SOLUTIONS

CERTIFICATE OF ANALYSIS

260904-899-NHS-4

Issued Oct 8, 2026

SAMPLE

# 5-AMINO

Prepared for **Aevum Plus** · Lot **AEV-AMQ50-20260828-01**

**PASS**

**ISO/IEC 17025:2017 ACCREDITED**

A2LA R243 · PJLA Testing #84351 · Zero recalls since 2016

181 W Huntington Dr, Suite 181, Monrovia, CA 91016 · (818) 808-9757

| BATCH / LOT | SAMPLE ID | MATRIX | PANELS RUN |
|---|---|---|---|
| AEV-AMQ50-20260828-01 | 260904-899-NHS-4 | Peptide | 3 |

| RECEIVED | ANALYZED | REPORTED | CLIENT |
|---|---|---|---|
| Sep 4, 2026 | — | Oct 8, 2026 | Aevum Plus |

## PEPTIDE PURITY

| ANALYTE | RESULT | UNIT | LIMIT / METHOD | STATUS |
|---|---|---|---|---|
| 5-AMINO — purity | 99 | % | HPLC-UV @ 274 nm | PASS |


## WATER ACTIVITY

| ANALYTE | RESULT | UNIT | LIMIT / METHOD | STATUS |
|---|---|---|---|---|
| Water activity | 0.31 | aw | < 0.65 | PASS |

## MICROBIALS

| ANALYTE | RESULT | UNIT | LIMIT / METHOD | STATUS |
|---|---|---|---|---|
| Yeast & Mold | Not Detected | | | PASS |
| Coliforms | Not Detected | | | PASS |
| E. Coli | Not Detected | | Not detected in 1 g | PASS |

## CHROMATOGRAM

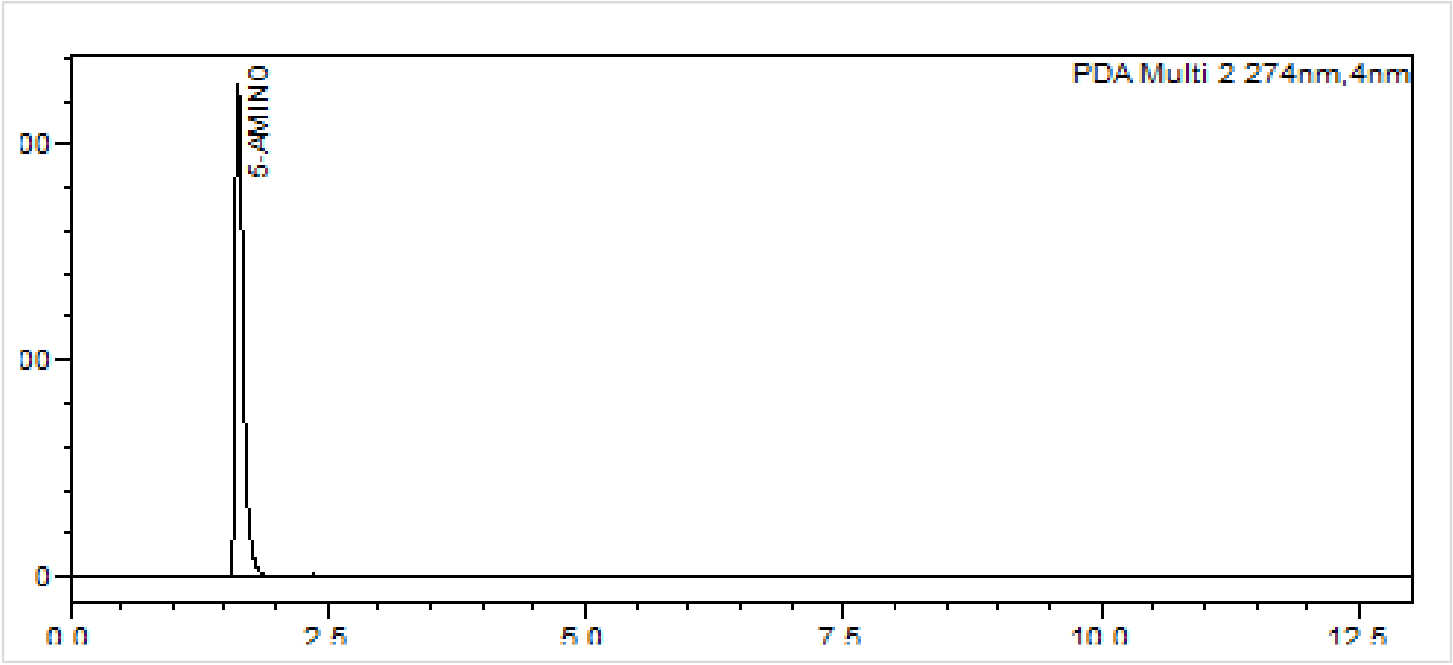


**PH SOLUTIONS LAB INC.**

Analysis performed in accordance with ISO/IEC 17025:2017. Results relate only to the sample as submitted. This certificate may not be reproduced except in full without the written approval of the laboratory. The online copy at the address beside is authoritative: if a printed COA disagrees with it, the online copy governs. Questions: info@phsolutionslab.com · (818) 808-9757.

SCAN TO VERIFY

www.phsolutionslab.com/c/eyJjIjoiMjYwOTA0LTg5OS1OSFMtNCIsInAiOiJBZXZ1bSBQbHVzIiwibCI6IkFFVi1BTVE1MC0yMDI2MDgyOC0wMSJ9.lwf2iCVldnbb9yFnWPgnY3x5GWv0-2EQ